EMX Series Multiframes

User Manual

© Copyright 2011 - 2021

EVERTZ MICROSYSTEMS LTD.

5292 John Lucas Drive Burlington, Ontario Canada L7L 5Z9

Phone: +1 905-335-3700


Sales: sales@evertz.com Fax: +1 905-335-3573
Tech Support: service@evertz.com Fax: +1 905-335-7571

Web Page: http://www.evertz.com

Version 1.6, Jan 2021

The material contained in this manual consists of information that is the property of Evertz Microsystems and is intended solely for the use of purchasers of the EMX Series Multiframes. Evertz Microsystems expressly prohibits the use of this manual for any purpose other than the operation of the EMX Series Multiframes. Due to on going research and development, features and specifications in this manual are subject to change without notice.

All rights reserved. No part of this publication may be reproduced without the express written permission of Evertz Microsystems Ltd. Copies of this manual can be ordered from your Evertz dealer or from Evertz Microsystems.



IMPORTANT SAFETY INSTRUCTIONS



The lightning flash with arrowhead symbol within an equilateral triangle is intended to alert the user to the presence of uninsulated "Dangerous voltage" within the product's enclosure that may be of sufficient magnitude to constitute a risk of electric shock to persons.



The exclamation point within an equilateral triangle is intended to alert the user to the presence of important operating and maintenance (Servicing) instructions in the literature accompanying the product.

- Read this information
- Keep these instructions.
- Heed all warnings.
- Follow all instructions.
- Do not use this apparatus near water
- Clean only with dry cloth.
- Do not block any ventilation openings. Install in accordance with the manufacturer's instructions.
- Do not install near any heat sources such as radiators, heat registers, stoves, or other apparatus (including amplifiers) that produce heat.
- Do not defeat the safety purpose of the polarized or grounding type plug. A polarized plug has two blades with one wider than other. A grounding type plug has two blades and a third grounding prong. The wide blade or the third prong is provided for your safety. If the provided plug does not fit into your outlet, consult an electrician for replacement of the obsolete outlet.
- Protect the power cord from being walked on or pinched particularly at plugs, convenience receptacles and the point where they exit from the apparatus.
- Only use attachments/accessories specified by the manufacturer
- Unplug this apparatus during lightning storms or when unused for long periods of time.
- Refer all servicing to qualified service personnel. Servicing is required when the apparatus has been damaged in any way, such as power-supply cord or plug is damaged, liquid has been spilled or objects have fallen into the apparatus, the apparatus has been exposed to rain or moisture, does not operate normally, or has been dropped.

WARNING

TO REDUCE THE RISK OF FIRE OR ELECTRIC – SHOCK, DO NOT EXPOSE THIS APPARATUS TO RAIN OR MOISTURE

WARNING

DO NOT EXPOSE THIS EQUIPMENT TO DRIPPING OR SPLASHING AND ENSURE THAT NO OBJECTS FILLED WITH LIQUIDS ARE PLACED ON THE EQUIPMENT

WARNING

TO COMPLETELY DISCONNECT THIS EQUIPMENT FROM THE AC MAINS, DISCONNECT THE POWER SUPPLY CORD PLUG FROM THE AC RECEPTACLE

WARNING

THE MAINS PLUG OF THE POWER SUPPLY CORD SHALL REMAIN READILY OPERABLE

INFORMATION TO USERS IN EUROPE

NOTE

This equipment with the CE marking complies with both the EMC Directive (89/336/EEC) and the Low Voltage Directive (73/23/EEC) issued by the Commission of the European Community.

Compliance with these directives implies conformity to the following European standards:

- EN60065 Product Safety
- EN55103-1 Electromagnetic Interference Class A (Emission)
- EN55103-2 Electromagnetic Susceptibility (Immunity)

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to the European Union EMC directive. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

INFORMATION TO USERS IN THE U.S.A.

NOTE

FCC CLASS A DIGITAL DEVICE OR PERIPHERAL

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

WARNING

Changes or modifications not expressly approved by Evertz Microsystems Ltd. could void the user's authority to operate the equipment.

Use of unshielded plugs or cables may cause radiation interference. Properly shielded interface cables with the shield connected to the chassis ground of the device must be used.



REVISION HISTORY

REVISION	<u>DESCRIPTION</u>	DATE
1.0	First Release	Feb 2011
1.1	Updated power supply specs	May 2013
1.2	Updated EMX1-FR	May 2014
1.3	Added EMX-FC information	Aug 2014
1.4	Some minor changes	Oct 2015
1.5	Updated electrical installation and service instructions	Dec 2020
1.6	Updated section 4.2 and 5.1.1 safety instructions	Jan 2021

Information contained in this manual is believed to be accurate and reliable. However, Evertz assumes no responsibility for the use thereof nor for the rights of third parties, which may be affected in any way by the use thereof. Any representations in this document concerning performance of Evertz products are for informational use only and are not warranties of future performance either expressed or implied. The only warranty offered by Evertz in relation to this product is the Evertz standard limited warranty, stated in the sales contract or order confirmation form.

Although every attempt has been made to accurately describe the features, installation and operation of this product in this manual, no warranty is granted nor liability assumed in relation to any errors or omissions unless specifically undertaken in the Evertz sales contract or order confirmation. Information contained in this manual is periodically updated and changes will be incorporated into subsequent editions. If you encounter an error, please notify Evertz Customer Service department. Evertz reserves the right, without notice or liability, to make changes in equipment design or specifications.



This page left intentionally blank



TABLE OF CONTENTS

1.	OVE	RVIEW	1
2.	INST	TALLATION	3
	2.1.	COOLING – EMX1-FR	4
		2.1.1. Fan Exhaust	4
	2.2.	COOLING - EMX3-FR	5
		2.2.1. Fan Exhaust	5
	2.3.	COOLING - EMX6-FR	5
		2.3.1. Fan Exhaust	5
	2.4.	MOUNTING	6
	2.5.	POWER	6
		2.5.1. Power Cord	6
		2.5.2. Power Supply Status Indicators	
		2.5.2.2. EMX3-FR and EMX6-FR	8
	2.6.	FRAME CONTROLLER	
		2.6.1. Configuring Basic Network settings	
3.	CDE	2.6.2. Ethernet Connection	
ა.			
	3.1.	ELECTRICAL	11
	3.2.	PHYSICAL	11
		3.2.1. Compliance	12
	3.3.	STATUS INDICATORS	12
	3.4.	PHYSICAL	13
	3.5.	MODULE CAPACITY	13
	3.6.	WEIGHT	13
4.	INST	TALLING AND REMOVING THE MODULES	15
	4.1.	ELECTRO STATIC DISCHARGE (ESD) PRECAUTIONS	15
	4.2.	RESTRICTED ACCESS AREA	15
	4.3.	INSTALLING THE MODULE REAR PLATES	15

EMX Series Multiframes



4.4.	. OPENING AND CLOSING THE FRONT PANEL	15
	4.4.1. EMX3 and EMX64.4.2. EMX1	
4.5.	. INSTALLING THE MODULES	
4.6.	. REMOVING THE MODULES	16
5. SEF	RVICING INSTRUCTIONS	17
5.1.	. INSTRUCTIONAL SAFEGUARDS	17
	5.1.1. IEC 60417-5041 Hot Surface	18
5.2.	. CHANGING THE FUSES (NOT APPLICABLE TO EXM1)	18
5.3.	. REPLACING THE POWER SUPPLY	18
Figures	;	
Figur Figur Figur Figur Figur	re 2-1: EMX1-FR Rear View	3
Tables		
Table	e 2-1: LED Status	8



1. OVERVIEW

The EMX series frames are designed to house the EMR series router, the EMC master controller and other high-density system products. This advanced rack frame design comes in three sizes. The EMX1-FR occupies 1RU rack space and can house up to 2 single-slot modules. The EMX3-FR occupies 3RU rack space and can house up to 5 single-slot modules of any combination of the EMR and EMC products. The EMX6-FR occupies 6RU rack space and can house up to 15 single-slot modules of the same products.

Special care was taken during the design process to ensure that the EMX1-FR, EMX3-FR and EMX6-FR frames meet the demanding needs of television studios today and have the sufficient flexibility to satisfy the emerging demands of the future. The EMX1-FR, EMX3-FR and EMX6-FR frames are designed with a high density capacity to conserve on precious equipment rack space. Care has been taken to ensure sufficient thermal relief for up to 140 W (EMX1-FR), up to 360 W (EMX3-FR) and 650 W (EMX6-FR) of processing power per frame, to meet the increasing power demands of future high speed processing cards. Hot swappable redundant switching power supplies and cooling fans allow power supply or fan replacement without compromising the integrity of critical signal paths. The EMX1-FR, EMX3-FR and EMX6-FR frames are available with auto ranging 100-240 VAC power supplies. The front loading design permits extraction of the power supplies and active modules from the front without compromising performance even at 3.0Gb/s. Thus, there is no need for time consuming re-cabling nor is there need to have access to the rear of the frame to replace or exchange modules.

The EMX1-FR, EMX3-FR and EMX6-FR frames can both accommodate a main and redundant frame controller (EMX-FC) to provide reference, Ethernet control and serial control for certain applications.

Features:

- Houses up to 2 (EMX1-FR), 5 (EMX3-FR) or 15 (EMX6-FR) single-slot processing modules
- Each slot has individually configurable inputs and outputs
- Front extractable modules, power supplies and fans
- Auto-ranging power supply that operates from 100-240VAC at 50/60 Hz
- Power supply and frame cooling fans are fully redundant and hot-swappable
- High-speed busing and control system provided for modular applications
- Slots available for main and redundant EMX-FC frame controllers, in EMX3-FR and EMX6-FR
- 140 W (EMX1-FR), 360 W (EMX3-FR) or 650 W (EMX6-FR) power supplies and cooling to support EMR and EMC modules
- Two BNCs for connecting two separate genlock references for modules equipped to take a frame reference input



This page left intentionally blank



2. INSTALLATION

The EMX1-FR, EMX6-FR and EMX3-FR frames use an EMX-FC frame controller which provides two network connections via RJ-45 connectors and two references via BNC connectors. The BNC labeled Ref 1 is the main reference and the BNC labeled Ref 2 is the backup reference. Figure 2-2 and Figure 2-3 show the rear of the EMX3-FR and EMX6-FR frames respectively.

The EMX3-FR and EMX6-FR frames have optional redundant frame controller configurations; however the EMX1-FR only houses one frame controller.




Figure 2-1: EMX1-FR Rear View

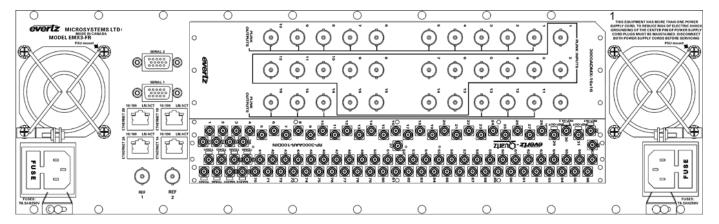


Figure 2-2: EMX3-FR Rear View



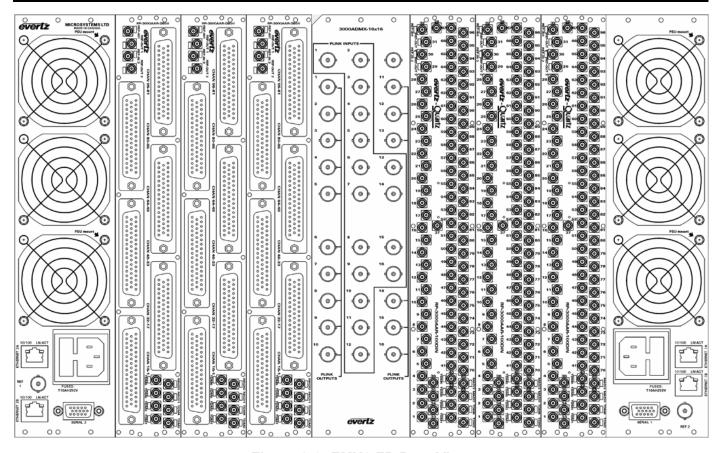


Figure 2-3: EMX6-FR Rear View

2.1. COOLING - EMX1-FR

The EMX1-FR frame is designed to ensure adequate cooling for up to 140 watts of processing power per frame. PSU's are cooled with their own internal fans. Adjacent equipment may be mounted immediately to the top and bottom of the EMX1-FR. Module cooling is provided by fans mounted to the front of panel of the frame.

2.1.1. Fan Exhaust

The power supply fans draw air in the front and exhaust out the back of the frame. The module fans draw in air from the front and exhaust out the right hand side of the frame.



CAUTION: To ensure adequate cooling, care should be taken to ensure that the fan inlets and exhaust openings are free of obstructions.



CAUTION: To ensure adequate cooling of modules, the front panel must always be securely mounted to the frame.

Page - 4 Revision 1.6



2.2. COOLING - EMX3-FR

The EMX3-FR is designed to ensure adequate cooling for up to 360 watts of processing power per frame. Fans at the front and rear of each power supply module accomplish forced air cooling. Adjacent equipment may be mounted immediately to the top and bottom of the EMX3-FR frame. Additional module cooling is provided by interior cooling channels to ensure that even fully loaded frames mounted vertically adjacent to each other will operate within the normal temperature range.

2.2.1. Fan Exhaust

The cooling fans for the power supplies, located at the front of the frame, draw air in the front and exhaust out the sides of the frame. The cooling fans for the modules, located at the rear of the frame, draw air in the front and the exhaust out the rear of the frame.



CAUTION: To ensure adequate cooling, care should be taken to ensure that the fan inlets and exhaust openings are free of obstructions.

2.3. COOLING - EMX6-FR

The EMX6-FR frame is designed to ensure adequate cooling for up to 650 watts of processing power per frame. Fans at the front and rear of each power supply module accomplish forced air cooling. Adjacent equipment may be mounted immediately to the top and bottom of the EMX6-FR. Additional module cooling is provided by interior cooling channels to ensure that even fully loaded frames mounted vertically adjacent to each other will operate within the normal temperature range.

2.3.1. Fan Exhaust

The cooling fans for the power supplies, located at the front of the frame, draw air in the front and exhaust out the sides of the frame. The cooling fans for the modules, located at the sides of the frame, draw air in the front and the exhaust out the left and right sides of the frame.



CAUTION: To ensure adequate cooling, care should be taken to ensure that the fan inlets and exhaust openings are free of obstructions.



2.4. MOUNTING

The EMX1-FR requires a 19" x 1.75" x 18.75" (483 mm x 45mm x 477mm) space, the EMX3-FR requires a 19" x 5.25" x 15.75" (483 mm x 133 mm x 400 mm) space and the EMX6-FR requires a 19" x 10.5" x 15.75" (483 mm x 260 mm x 400 mm) space. To securely fasten the frame to the equipment rack, make sure that all four mounting screws on each mounting rail are tightened securely.



Note: The EMX6-FR, EMX3-FR and EMX1-FR have front mounted cooling fans and require that the area below is flush so that there is sufficient room to open the frame completely to be able to remove the modules.

After the unit has been installed in a rack, all cards in the frame should be checked to ensure they are fully seated within the frame. This is best accomplished by simply pushing (simultaneously, with moderate force) on each card's top and bottom insertion/extraction levers. This step should be repeated any time the frame is shipped, or relocated within a facility.

2.5. POWER

2.5.1. Power Cord

Power should be applied by connecting a 3-wire grounding type power supply cord to the power entry module on the rear panel of each power supply. For use in North America, the power cord should be a minmum 14AWG wire, type SVT marked VW-1, maximum 2.5m in length. For use outside North America use a power cord approved for the country of use with a minimum 1.00mm² wire size.



CAUTION – To reduce risk of electric shock, grounding of the ground pin of the mains plug must be maintained.

Page - 6 Revision 1.6



2.5.2. Power Supply Status Indicators

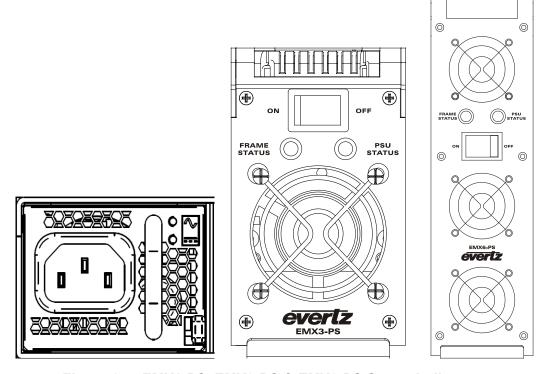


Figure 2-4: EMX1-PS, EMX3-PS & EMX6-PS Status Indicators



2.5.2.1. EMX1-FR

EMX1-FR power supplies have 2 LEDs which are located on the rear side of the frame, showing the status of each supply. Top LED is green and indicated AC power is on or off. Bottom LED is bi-colored: green and yellow. This indicated DC power presence or fault situations. For the position of LEDs see Figure 2-4. The following table shows different LED states:

Operating Condition	LED Signaling	
AC LED		
AC Line within range	Solid Green	
AC Line UV condition	Off	
DC LED		
12V DC		
Over temperature shutdown		
Output over voltage shutdown (12V DC)	Solid Yellow	
Output over current shutdown (12V DC)		
PSU Fan Error (>15%)		
Over temperature warning	Blinking Yellow/Green (2:1)	
Minor fan regulation error (>5%, <15%)	Blinking Yellow/Green (1:1)	
12V DC Good	Solid Green	

Table 2-1: LED Status

2.5.2.2. EMX3-FR and EMX6-FR

Each power supply has two status indicator LEDs. The green PSU STATUS LED indicates the health of the local power supply and its fans. The green PSU STATUS LED will be On under normal conditions. The FRAME STATUS LED indicates the health of the entire frame and is operated by the frame status bus of the frame. The red FRAME STATUS LED will be Off under normal conditions and On when there are Frame Status Fault conditions.

If one of the power supplies malfunctions, (power cord disconnected, power switch is off, fuse is blown, rear fan is stopped, etc,) then its green PSU STATUS LED will go Off, and the red FRAME STATUS LED on both power supplies will turn On and the Frame Status fault will be signaled to the Frame status buss. The PSU STATUS LED on the power supply that is functioning will remain On.

Page - 8 Revision 1.6



2.6. FRAME CONTROLLER

To successfully install the EMX-FC, you will require the following:

- 1. Unused IP address on the network or a DHCP server.
- 2. Evertz serial cable.

Before handling the card it is important to minimize the potential effects of static electricity. It is therefore recommended that an ESD strap be worn.

Before inserting the card, connect the serial cable to the board using the serial cable provided as shown in Figure 2-5. Now insert the FC card into the dedicated front slot ensuring the card lines up with the slot runners on the bottom and the top of the chassis. Push the card **firmly** into the slot ensuring that when it mates with the rear card it has been firmly pushed into a seated position. Do not connect any cables to the rear card (failure to do this could cause unwanted network issues) until the initial configuration has been completed.

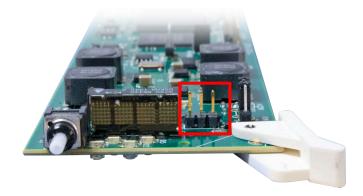


Figure 2-5: Serial Connection

Connect the 9-pin D-type end of the serial cable to the serial port of your computer.

Open Tera Term (if using Windows XP or older operating systems, open Hyper Terminal) to make the required changes to the IP address on the card. Set the required Baud rate to 115200 and use username *customer* and password *customer* to login.




Figure 2-6: Tera Term Main Menu



2.6.1. Configuring Basic Network settings

To make changes to the IP address select **Network Setup**. Set the IP address of the B Network as well as the **Netmask** and the **Gateway**. Make the same changes for the IP address and Gateway of Network A and C as required. When done **Exit** (X) the Network Setup and **Save and Exit** (X) from the Main Menu to ensure all changes are saved. Reboot the card to ensure the changes take effect.

```
Network Configuration
                (EMX-FC revB v4.11 et.12507)
  B network is enabled
 BCM switch (FCC1)
MACO
                                       : 00:02:c5:15:4c:a7
                                         192.168.10.54
            ip address
           netmask address
                                       : 255.255.255.0
 C network is enabled
MI: Inter-FC (FCC2)
           MAC1
                                       : 00:02:c5:15:4c:a8
                                       : 192.168.11.13
: 255.255.255.0
            ip address
           netmask address
 A network is enabled
TCP proxy (FCC3)
MAC2
                                       : 00:02:c5:15:4c:a9
                                         0.0.0.0
           ip address
                                       : 0.0.0.0
           netmask address
           broadcast address
                                      : 192.168.10.255
           gateway
                                       : 192.168.10.1
(1) Enable Network B
(2) Set IP Address B
(3) Set Netmask B
(4) Enable Network C
(5) Set IP Address C
 (6) Set Netmask C
(7) Enable Network A
(8) Set IP Address A
(9) Set Netmask A
(10) Set Gateway
($) Save and Exit
(X) Exit
> [
```

Figure 2-7: Tera Term Network Configuration

2.6.2. Ethernet Connection

For the EMX6 and EMX3 frames, ensure the Ethernet connection is made through Ethernet port 1B. For the EMX1 frame, ensure the Ethernet connection is made through Ethernet port 1.

Page - 10 Revision 1.6



3. SPECIFICATIONS

3.1. ELECTRICAL

EMX6-FR:

AC Mains Input: Auto ranging, 100 ⇔ 240 VAC, 50/60 Hz

Max Operating Current: 9.5 A (@ 115 VAC nominal), 4.0 A (@ 220 VAC nominal)

Max Power Consumption: 850 W

Max Module Load: 650 W (40 W per slot)

Power Supply Configuration: 1 supply standard, optional redundant supply requires separate inlet

Connector: IEC 60320 - 1 per power supply

EMX3-FR:

AC Mains Input: Auto ranging, 100 ⇔ 240 VAC, 50/60 Hz **Max Operating Current:** 4.6 A (@ 100 V/60Hz), 1.85A (@ 240 V/50Hz)

Max Power Consumption: 450 W

Max Module Load: 360 W (24 W per slot)

Power Supply Configuration: 1 supply standard, optional redundant supply requires separate inlet

Connector: IEC 60320 - 1 per power supply

EMX1-FR:

AC Mains Input: Auto ranging, 100 ⇔240 V AC, 50/60Hz **Max Operating Current:** 8.5 A (@ 100V/60Hz), 3.0 A (@ 240V/50Hz)

Max Power Consumption: 600 W

Max Module Load: 140 W (70 W per slot)

Power Supply Configuration: 1 supply standard, optional redundant supply required separate inlet

Connector: IEC 60320 – 1 per power supply

3.2. PHYSICAL

EMX6-FR:

Height:10.5" (266mm)Width:19.0" (483mm)Depth:15.75" (400mm)

Module Capacity: 15 single slot EMR series modules

Weight Approx.: 34.8lbs (15.8kg) with 2 power supplies, no slots occupied

64.0lbs (29kg) with 2 power supplies, all slots occupied

EMX3-FR:

Height:5.25" (133mm)Width:19.0" (483mm)Depth:15.75" (400mm)

Module Capacity: 5 single slot EMR series modules

Weight Approx.: 17.4lbs (7.9kg) with 2 power supplies, no slots occupied

32.0lbs (14.5kg) with 2 power supplies, all slots occupied



EMX1-FR:

Height:1.75" (45 mm)Width:19.0" (483 mm)Depth:18.75" (477 mm)

Module Capacity: 2 single slot EMX series modules

Weight: 15 lbs (6.8kg) with 2 power supplies, no slots occupied

22.0lbs (10kg) with 2 power supplies, all slots occupied

3.2.1. Compliance

EMX6-FR:

Safety: CSA Listed to CSA C22.2 No. 60065-03, UL 60065-03

IEC 60065-(2001-12) 7th Edition

Complies with CE Low voltage Directive 93/68/EEC

EMC: Complies with FCC part 15, class A

Complies with EU EMC directive 89/336/EEC

EMX3-FR:

Safety: CSA Listed to CSA C22.2 No. 60065-03, UL 60065-03

IEC 60065-(2001-12) 7th Edition

Complies with CE Low voltage Directive 93/68/EEC

EMC: Complies with FCC part 15, class A

Complies with EU EMC directive 89/336/EEC

EMX1-FR:

Safety: CSA Listed to CAN/CSA-C22.2 No. 60950-1-07, Amendment

1:2011(MOD)

ANSI/UL Std. No. 60950-1-2011

Complies with CE Low voltage Directive 2004/108/EC

EMC: Complies with FCC part 15, class A

Complies with EU EMC directive 89/336/EEC

3.3. STATUS INDICATORS

PSU status LED

Local Error/Failure LED

Page - 12 Revision 1.6



3.4. PHYSICAL

Dimensions:

EMX3-FR: 19" W x 5.25" H x 15.75" D

(483mm W x 133mm H x 400mm D)

EMX6-FR: 19" W x 10.5" H x 15.75" D

(483mm W x 266mm H x 400mm D)

EMX1-FR: 19.0" W x 1.75" H x 18.75" D

(483mm W x 45mm H x 477mm D)

Temperature: 0-40°C

3.5. MODULE CAPACITY

EMX1-FR: 2 single slot modules EMX3-FR: 5 single slot modules EMX6-FR: 15 single slot modules

3.6. WEIGHT

EMX1-FR: 22.0lbs (10kg) Full, 15lbs (6.8kg) Empty **EMX3-FR:** 32lbs (14.5kg) Full, 17.4lbs (8kg) Empty **EMX6-FR:** 64lbs (29g) Full, 34.8lbs (16kg) Empty



This page left intentionally blank



4. INSTALLING AND REMOVING THE MODULES

4.1. ELECTRO STATIC DISCHARGE (ESD) PRECAUTIONS



All semiconductor devices are sensitive to ESD. To prevent any damage or degradation on components of the product caused by ESD, observe these precautions when installing or removing modules from the frame.

- 1. Discharge static from your body. Wear a grounded anti-static wrist or heel strap, to discharge the static voltage from your body.
- 2. Use a Safe Work Area. Avoid handling modules in areas that have a floor or work surface covering capable of generating a static charge. Also nothing capable of generating or holding a static charge should be allowed in the work area.
- 3. Handle ESD sensitive modules carefully. Do not slide modules over any surface. Do not touch exposed connector pins. Pick-up modules by the edges of the modules, never by touching exposed leads.
- 4. Transport and store sensitive components or assemblies in a static-protected bag or container.

4.2. RESTRICTED ACCESS AREA

This equipment is intended only for use in a restricted access area.

A restricted access area is defined as an area accessible only to skilled persons and instructed persons with the proper authorization.

4.3. INSTALLING THE MODULE REAR PLATES

Each module is shipped with a matching rear panel plate which houses the connectors appropriate for the module. When installing a rear plate, locate the desired slot position where you wish to install the rear plate. Make a note of the slot number where you are installing the rear plate. Orient the plate so that the labeling is visible when the plate is installed. Loosely fasten the plate to the extrusions using the mounting screws provided, beginning with the top screw. You will tighten the screws after the main module is installed.

4.4. OPENING AND CLOSING THE FRONT PANEL



The front panel is used as a fire enclosure. The door should be kept closed except when servicing the equipment.



4.4.1. EMX3 and EMX6

In order to insert or remove modules you will have to open the front panel. Turn the two captive screws located on the front panel counter clockwise several turns until they release completely from the front extrusions. Carefully lower the front panel door so that the front edge of the door is lower than the rear of the door.

When closing the door, make sure that the thumbscrews are properly finger tightened. If the frame is operated in environments subject to excessive vibration such as mobile trucks, you may tighten the screws carefully with a screwdriver. Be careful not to over tighten as the thumbscrew head may twist off.

4.4.2. EMX1

In order to insert or remove modules you will have to remove the front panel. Turn the two captive screws located on the front panel counter clockwise several turns until they release completely from the front extrusions. Pull the front panel from the frame so it is completely removed.

When closing the door, make sure that the thumbscrews are properly finger tightened. If the frame is operated in environments subject to excessive vibration such as mobile trucks, you may tighten the screws carefully with a screwdriver. Be careful not to over tighten as the thumbscrew head may twist off.

4.5. INSTALLING THE MODULES

For the EMX6-FR, orient the module vertically such that the white card ejector is on the bottom. For the EMX1-FR and the EMX3-FR, orient the module horizontally such that the white card ejector is to the right. In both cases, align the card with the card guide corresponding to the slot number where you installed the rear panel plate. Carefully slide the module into the frame and press it completely into the rear panel connectors. Make sure that the connectors are fully seated in the rear panel. When this is done, close the front panel and then tighten the screws that hold the rear panel in place.

4.6. REMOVING THE MODULES

Press the card ejector down to release the module. Grasp the card using the card ejector and pull the module out from the frame. As the card ejector goes past the front extrusion, you will have to pull it with slightly more force. Carefully place the module in a safe place, free from static discharge.

Page - 16 Revision 1.6



5. SERVICING INSTRUCTIONS



CAUTION – These servicing instructions are for use by qualified service personnel only. To reduce risk of electric shock do not perform any servicing instructions in this section of the manual unless you are qualified to do so.



CAUTION – Equipment for use only in locations where children not likely to be present.



CAUTION – Danger of explosion if battery incorrectly replaced, replace only with the same or equivalent type recommended by the manufacturer. Dispose of used batteries according to manufacturer instructions or local ordinance.

ATTENTION: IL Y A RISQUE D'EXPLOSION SI LA BATTERIE EST REMPLACÉE PAR UNE BATTERIE DE TYPE INCORRECT. METTRE AU REBUT LES BATTERIES USAGÉES CONFORMÉMENT AUX INSTRUCTIONS.



CAUTION – To reduce the risk of electric shock, grounding of the ground pin of the mains plug must be maintained.

5.1. INSTRUCTIONAL SAFEGUARDS

Each EMX series device should have the following warning labels attached as instructional safeguards.

5.1.1. IEC 60417-5041 Hot Surface

The flat surface with waved line symbol is intended to alert the user that surface may be hot and should not be touched without taking care.



CAUTION - HOT SURFACE

Do Not Touch



5.1.2. The IEC 60417-6042 Lightning Flash Symbol

The lightning flash with arrowhead symbol within an equilateral triangle is intended to alert the user to the presence of uninsulated "Danger voltage" within the product's enclosure that may be of sufficient magnitude to constitute a risk of electric shock to persons.



CAUTION - SHOCK HAZARD

5.1.3. IEC 60417-6172 Multiple Power Sources Symbol

The multiple power source symbol with multiple power cords is intended to alert the users that all power sources should be disconnected to avoid shock hazards



CAUTION - DISCONNET ALL POWER SOURCES

5.2. CHANGING THE FUSES (NOT APPLICABLE TO EXM1)



Check that the line fuse is rated for the correct value marked on the rear panel. Never replace with a fuse of greater value.

The fuse holder is located inside the power entry module. To change the fuses, pull out the fuse holder from the power entry module using a small screwdriver. The fuse holder contains two fuses, one for the line and one for the neutral side of the mains connection. Pull out the blown fuse and place a fuse of the correct value in its place. The correct fuse rating is marked on the rear panel near the power entry module.

Fuse Rating: 10 Amps, 250 Volt ceramic time delay, 5 x 20 mm

5.3. REPLACING THE POWER SUPPLY

Each power supply is a complete assembly and includes the power supply cooling fan and one frame cooling fan. In the event that the power supply or one of the fans malfunctions, you will need to replace the power supply assembly with a spare one while the failed assembly is being repaired.

Page - 18 Revision 1.6





Do not run the frame for extended periods of time with one of the power supplies removed or with the door open. Proper cooling of the frame requires both power supplies to be inserted into the frame, or one power supply and a power supply fan module.

The EMX3-FR & EMX6-FR power supplies are hot swappable and can be easily replaced from the front without interrupting the signal integrity of the frame. Each power supply is capable of supplying full power to the frame by itself, however we recommend running with both supplies powered for power redundancy. In the case of the EMX6-FR, the redundant power supply is required to provide adequate cooling to the frame so it is always recommended.

On EMX3-FR frames with only one power supply, a blank power supply fan module with cooling fan (properly rated for the wattage of the power supply) **must be** inserted into the second power supply space. The blank power supply fan module contains a module cooling fan sufficient to cool the maximum power dissipation of the frame and baffles to maintain proper airflow within the frame.

The power supply is secured into the frame by a machine screw through the rear panel. This screw must be removed before the power supply can be extracted from the front.



To reduce risk of electric shock you must replace the mounting screw after replacing the power supply.

To replace the power supply the following procedure should be used for the EMX6-FR and EMX3-FR.

- 1. Turn off the power supply switch.
- 2. Unplug the power supply
- 3. From the rear of the frame locate the power supply mounting screw. This screw is the top right screw holding the fan guard in place, and is indicated by the legend

PSU Mount

- 4. Remove the power supply mounting screw.
- 5. Open the front door of the frame and pull the power supply out of the frame.
- 6. Reinsert the new power supply into the frame taking care that it is properly aligned with the card guides. Press firmly to make sure that the power supply is fully seated into the rear panel connector.
- 7. Reinstall the power supply mounting screw from the rear of the frame.
- 8. Plug in the new power supply power cord
- 9. Turn on the power switch for the power supply. After a few seconds you should see the PSU STATUS LED come on indicating that the power supply is working correctly.
- 10. Once you have confirmed the power supply is working correctly, close the front door of the frame.

To replace the power supply the following procedure should be used for the EMX1-FR.

- 1. Turn off the power supply switch
- 2. Remove AC power cable

EMX Series Multiframes



- 3. From the front of the frame, locate the power supply locking tab. Releasing this tab will allow the PSU to be removed from the frame.
- 4. Release the power supply locking tab.
- 5. Remove the Power Supply from the frame.
- 6. Reinsert the new power supply into the frame taking care that it is properly aligned with the card guides. Press firmly to make sure that the power supply is fully seated into the rear panel connector.
- 7. Turn on the power switch for the power supply. After a few seconds you should see the PSU STATUS LED come on indicating that the power supply is working correctly.

End of document

Page - 20 Revision 1.6